




Certificate of Analysis

SALSA® MLPA® Probemix P088 Oligodendroglioma 1p-19q

Catalogue #	P088-025R, P088-050R, P088-100R	
Product name	Probemix P088 Oligodendroglioma 1p-19q	
LOT	C2-0918	
	25, 50, or 100 reactions.	
Shipping conditions	Dry ice or cooling elements.	
	Store upon arrival between -25°C and -15°C.	
	Expiration date: September 2023, when stored at recommended conditions. This product should not be frozen/thawed more than 25 times.	
Use	This product has been developed to determine the DNA copy number status of the 1p and 19q chromosomal arms, and to detect the mutations p.R132H and p.R132C in the <i>IDH1</i> gene and p.R172K and p.R172M in the <i>IDH2</i> gene. This probemix is designed for use only in combination with SALSA MLPA reagent kits and Coffalyser.Net as described in the MLPA General Protocol.	
Quality control specifications	<ul style="list-style-type: none"> - Sufficient distance between peaks, absence of extra or shoulder peaks, and completeness of hybridisation of each individual probe, as tested on Applied Biosystems 3130 and Beckman/SCIEX GeXP sequencers. - Standard deviation of each individual probe ≤ 0.10, when tested on 23 different DNA samples of healthy individuals, extracted by various methods. - Each individual probe meets reaction-specific criteria when tested on a single DNA sample under various experimental conditions. - No DNA controls result in only five major peaks shorter than 121 nucleotides (nt): four Q-fragments at 64, 70, 76 and 82 nt, and one 19 nt peak corresponding to the unused portion of the fluorescent PCR primer. Non-specific peaks longer than 121 nt AND with a height <25% of the median of the four Q-fragments are not expected to affect MLPA reactions when sufficient (50-250 ng) sample DNA is used. 	Test result
		PASS

None of the ingredients are derived from humans, animals, or pathogenic bacteria. Based on the concentrations present, none of the ingredients are hazardous as defined by the Hazard Communication Standard. **A Safety Data Sheet (SDS) is not required for these products:** none of the preparations contain dangerous substances (as per Regulation (EC) No 1272/2008 [EU-GHS/CLP] and amendments) at concentrations requiring distribution of an SDS (as per Regulation (EC) No 1272/2008 [EU-GHS/CLP] and 1907/2006 [REACH] and amendments). If spills occur, clean with water and follow appropriate site procedures.

More information: www.mlpa.com; www.mlpa.eu

	MRC-Holland bv; Willem Schoutenstraat 1 1057 DL, Amsterdam, The Netherlands
E-mail	info@mlpa.com (information & technical questions); order@mlpa.com (orders)
Phone	+31 888 657 200

Certificate of Analysis

SALSA MLPA Probemix P088-C2 Oligodendroglioma 1p-19q sample picture

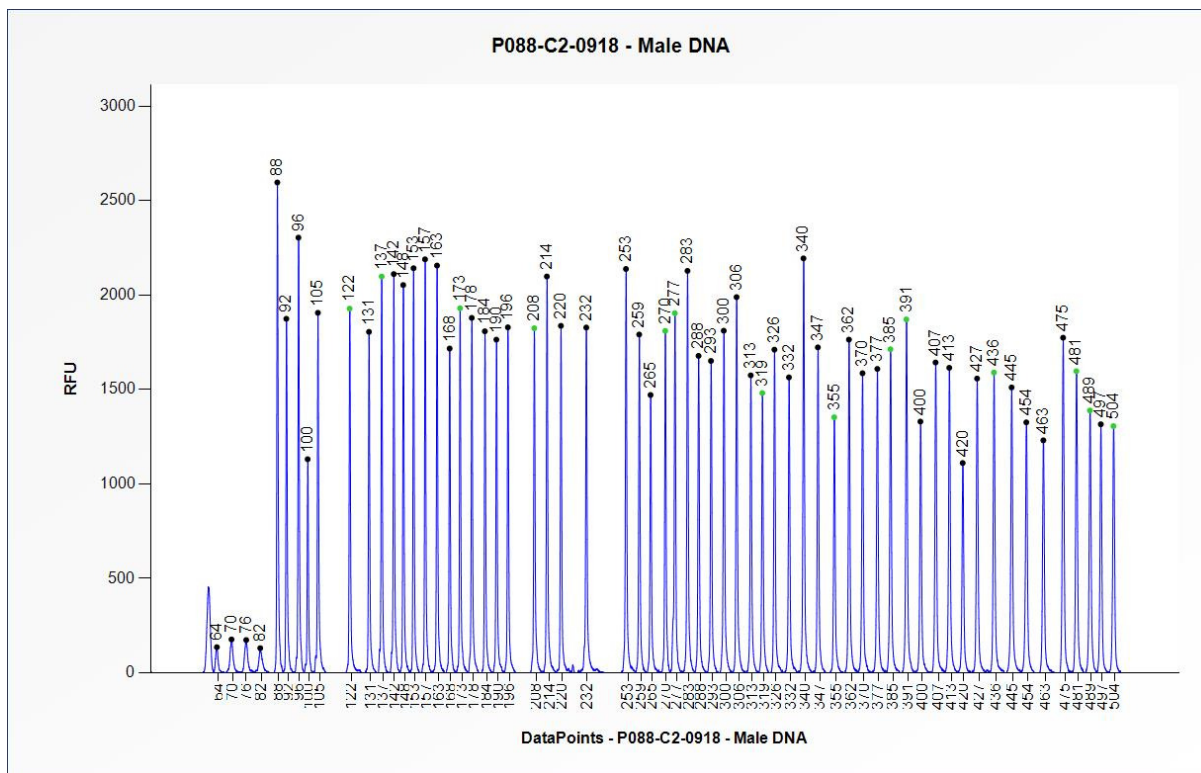


Figure 1. Capillary electrophoresis pattern from a sample of approximately 50 ng human male control DNA analysed with SALSA MLPA Probemix P088 Oligodendroglioma 1p-19q (C2-0918).

Certificate of Analysis

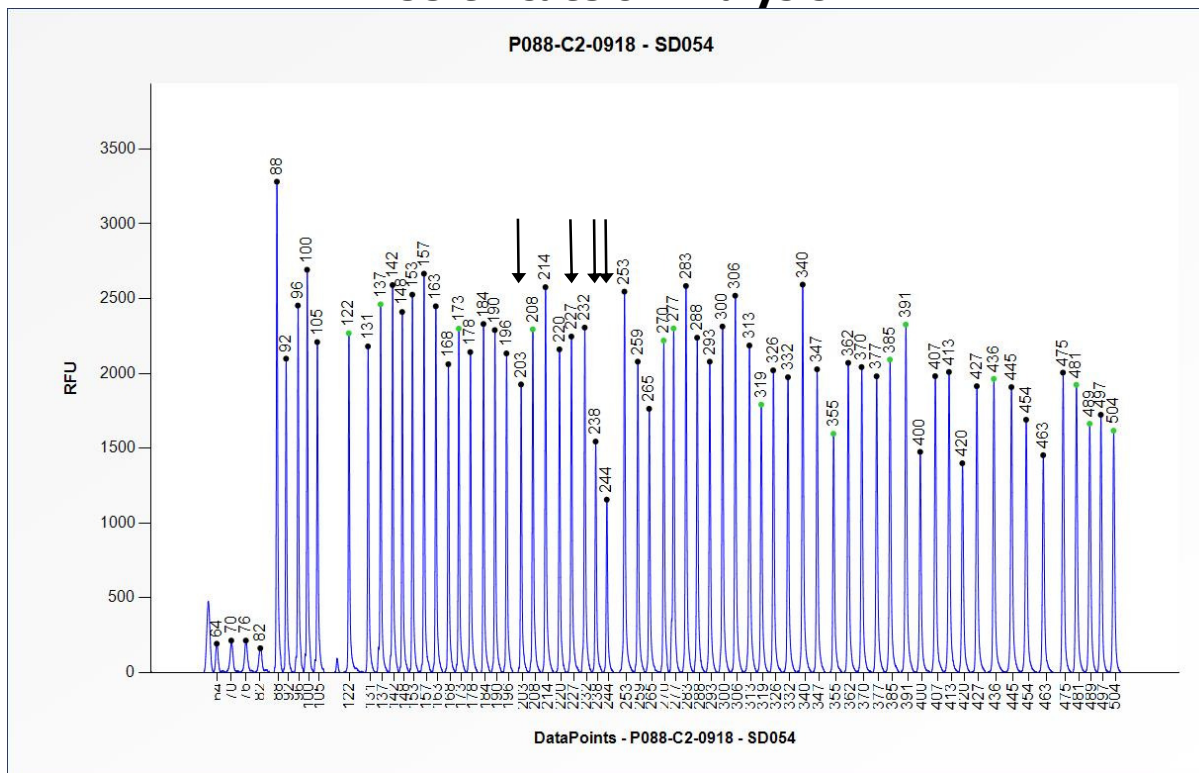


Figure 2. Capillary electrophoresis pattern from SALSA Binning DNA SD054-S01 (approximately 50 ng) analysed with SALSA MLPA Probemix P088 Oligodendroglioma 1p-19q (C2-0918). The location of the IDH1 mutation specific probe p.R132H at 203nt and p.R132C at 227nt, and the location of the IDH2 mutation specific probe p.R172K at 238nt and p.R172M at 244nt are indicated.

This lot was certified by MRC-Holland on 04 December 2018.

This certificate is a declaration of analysis at the time of the manufacturing process. All assays were run in compliance with manufacturer's instructions for use.

Implemented changes in the COA

Version 01 – 04 December 2018 (04)

- Not applicable, new document.